



Talisman Flotta Terminal

OIW EX1000 & Laboratory
Correlation

Data Supplied Courtesy Of
Talisman UK




March 2007

Average Difference for Month= 1.0039PPM




169 Sample March 07

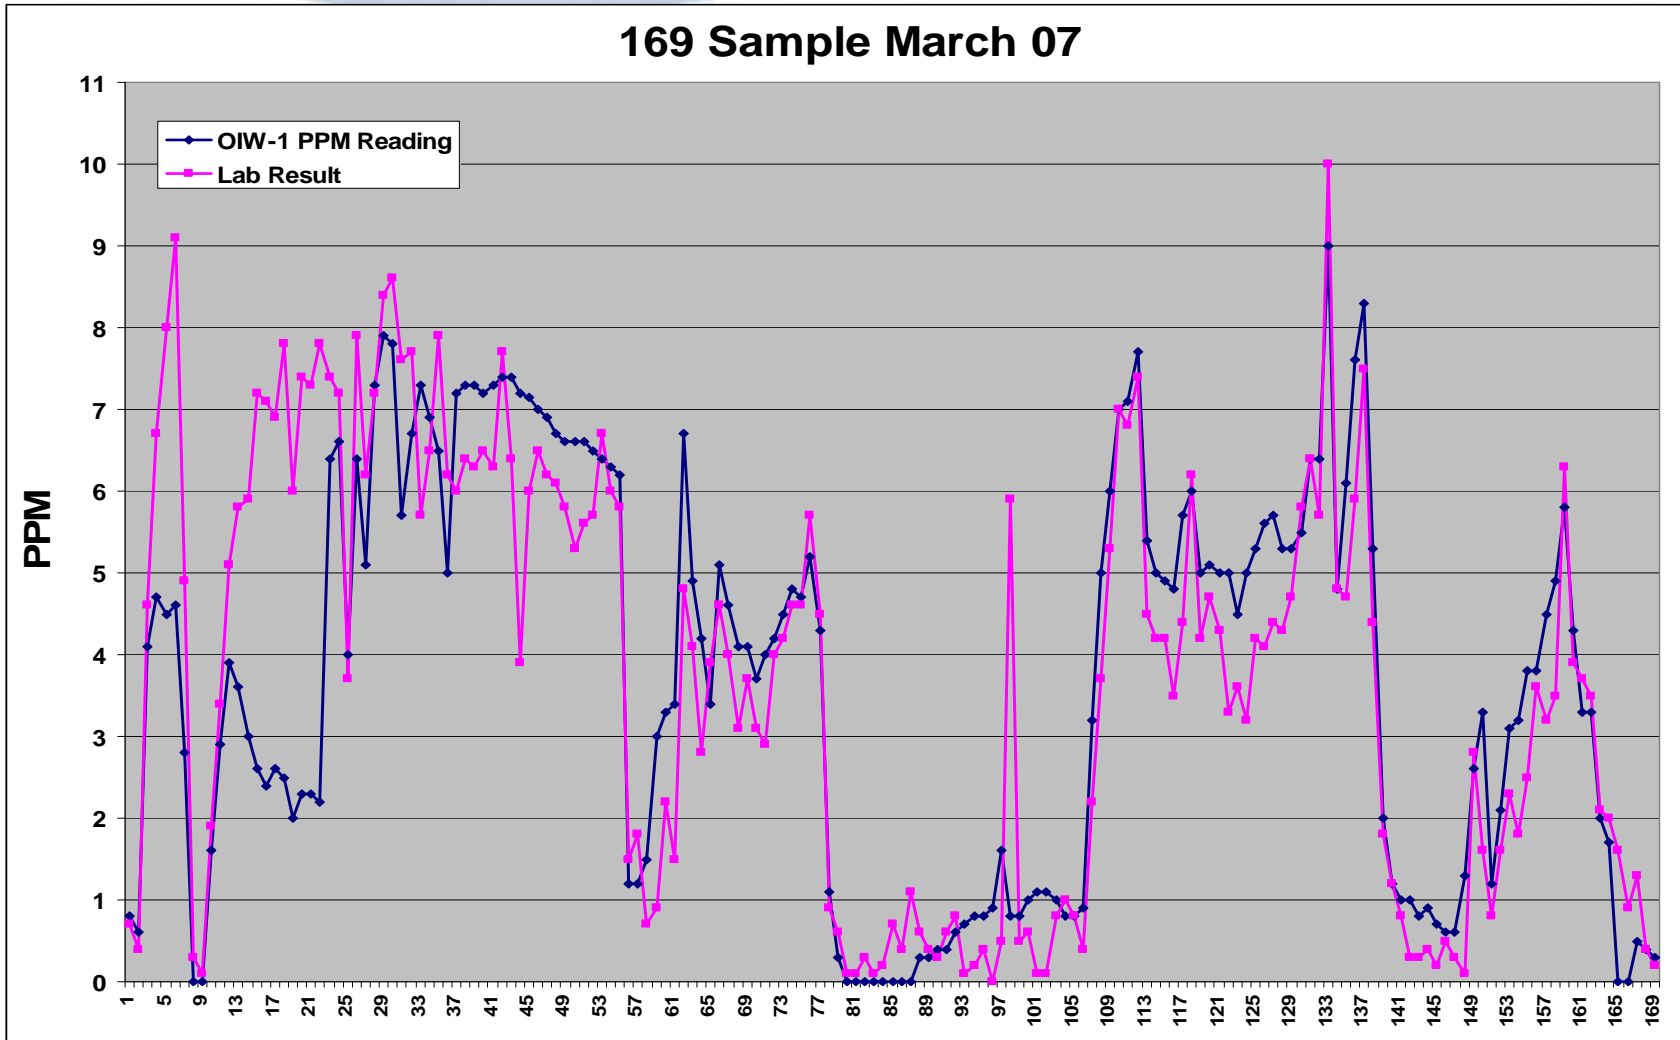



April 2007

Average Difference for Month= 0.8345PPM

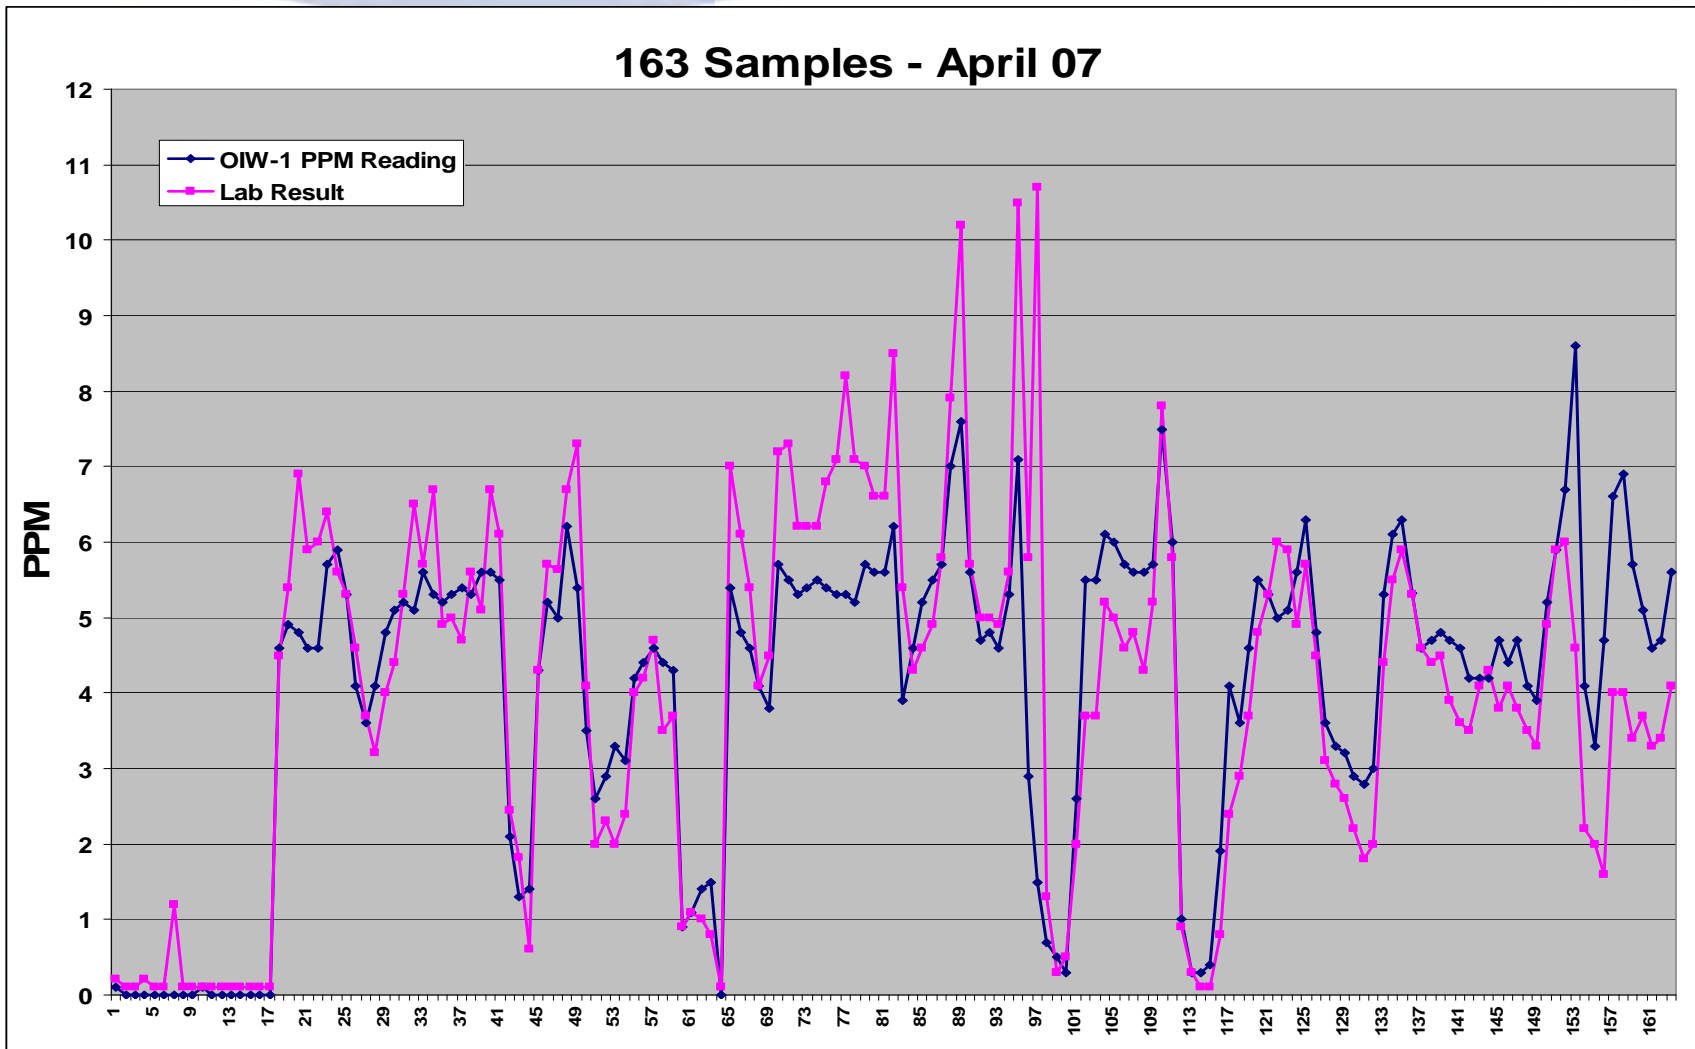


May 2007

Average Difference for Month= 0.8591PPM



179 Samples - May 07

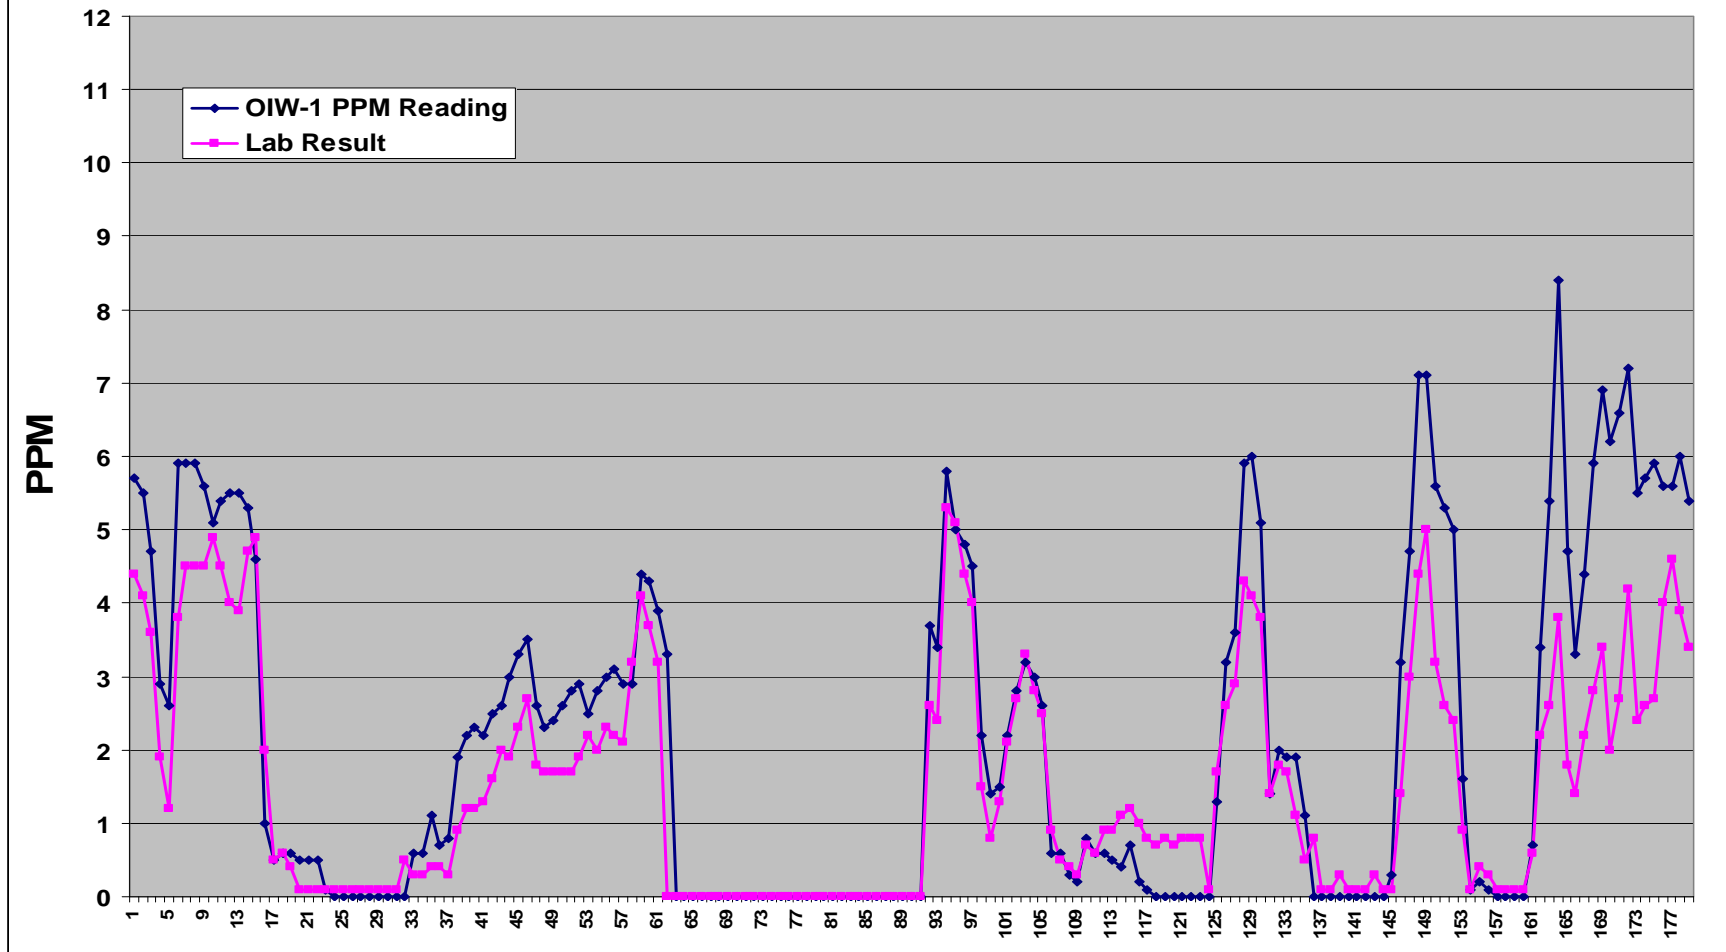

December 2007

Average Difference for Month= 0.34PPM

